# O2MATIC QUICK GUIDE

Get started quickly with O2matic




Applies to O2matic OMC PC-100 & PRO 100 with software version 1.6.2

## Setup a patient

1. Turn on the device by holding the ON/OFF button for 3 seconds.

2. Apply the Nonin sensor on the finger of the patient.

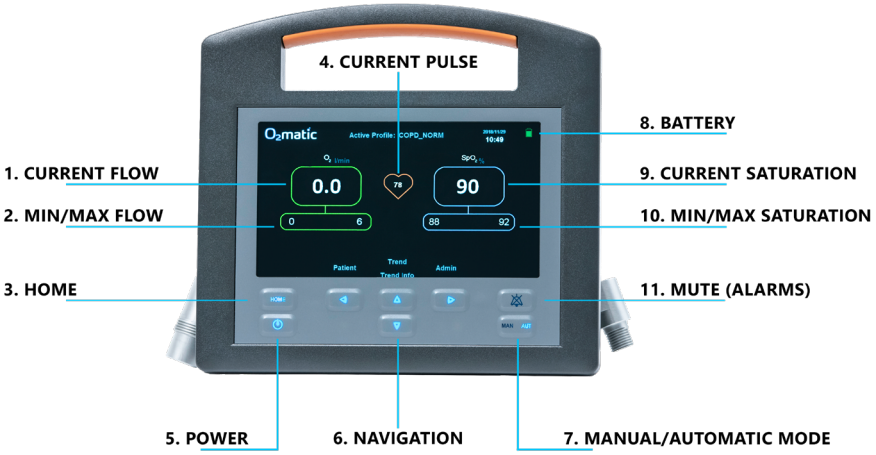3. Apply mask or nasal catheter.

**NOTE**: Make sure the switch on the back of the device is turned on. O2matic PRO will turn on with the latest saved settings.


## Patient data

Press "Trend Info" to see an average of the last 24 hours.

Press "Trend" to see a graph from the last hour - see fig. 1.

Change the interval on the trend graph by pressing the right and left buttons.

## Change patient or profile

**1.** Press "Patient".

**2.** Check if the profile settings are correct - See figure 2.

**3.** You are now presented with the following options:

**a)** New Patient - Create a new patient. The device will go through all of the settings for setting up a patient and finally creating it.

Select the up / down arrow keys to change settings and the left / right arrow keys to go back / forward in the profile creation process.

**b)** Select profile - Change the selected treatment profile. Select one of the default profiles created. New profiles can be created in the Admin menu.

**c)** Customize profile - Customize the selected treatment profile to the indivi dual patient. Added changes do not affect the default treatment profiles - See Figure 2.

**d)** Location - Add a location note, e.g. "Room 2" or "Bed 3" to make it easy to keep track of where your device belongs. The note can be seen at the bottom left

**NOTE:**
The "HOME" button always allows you to return to the home screen.
You can mute the alarm for 2 minutes by pressing the mute button.

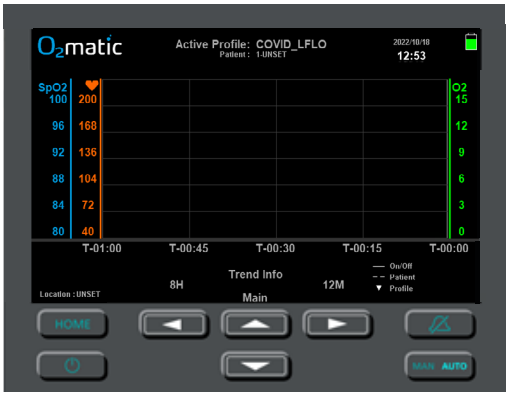


Figure 1 - Trend overview


Figure 2 - Customize profile

| PROFILE | SUITABLE FOR |
|---|---|
| | |
| **SpO2**: | |
| **Flow:** | |
| | |
| **SpO2**: | |
| **Flow:** | |
| | |
| **SpO2**: | |
| **Flow:** | |
| | |
| **SpO2**: | |
| **Flow:** | |
| **WALKING** | |
| **SpO2**: 90 - 94% | Used for 6 minutes walking test and other mobility tests. Should be attached to a rollator and run in battery mode. Adjusts oxygen flow faster. |
| **Flow:** 0 - 15 l/min | |

**Caution**
Max flow to oxygen sensitive patients should be assessed individually.